



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSA-0031
Location:	STAFFORD TOWNSHIP P.D.	
Calibration File No.:	01384	Calib. Date: 12/11/2017
Certification File No.:	01385	Calib. No.: 00031
Linearity File No.:	01386	Cert. Date: 12/11/2017
Solution File No.:	01397	Cert. No.: 00026
Sequential File No.:	01397	Lin. Date: 12/11/2017
		Lin. No.: 00026
		Soln. Date: 02/17/2018
		Soln. No.: 00194
		File Date: 02/17/2018

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0015
Solution Control Lot:	17200	Expires: 06/28/2019
		Bottle No.: 1066

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:53S		
Control 1 EC	0.099%	02:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	02:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:54S		
Control 2 EC	0.100%	02:54S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:55S		
Control 3 EC	0.099%	02:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MACFARLANE

First Name: ROBERT

MI: S

Signature: _____

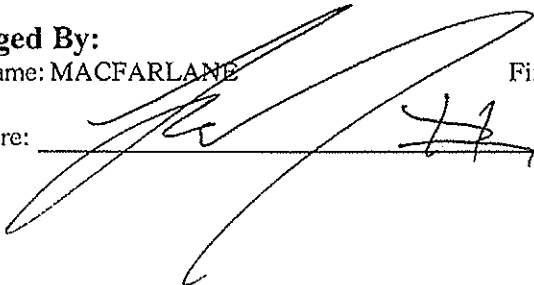

#110

Badge No.: 110

Date: 02/17/2018