

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSA-0031
Location:	STAFFORD TOWNSHIP P.D.	
Calibration File No.:	01494	Calib. Date: 05/15/2019
Certification File No.:	01495	Calib. No.: 00034
Linearity File No.:	01496	Cert. Date: 05/15/2019
Solution File No.:	01514	Cert. No.: 00029
Sequential File No.:	01514	Lin. Date: 05/15/2019
		Lin. No.: 00029
		Soln. Date: 07/17/2019
		Soln. No.: 00219
		File Date: 07/17/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0014
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 0534

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:49D		
Control 1 EC	0.099%	22:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:50D		
Control 2 EC	0.099%	22:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	22:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:51D		
Control 3 EC	0.099%	22:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: 4

First Name: JOSEPH

MI: R

Signature: _____

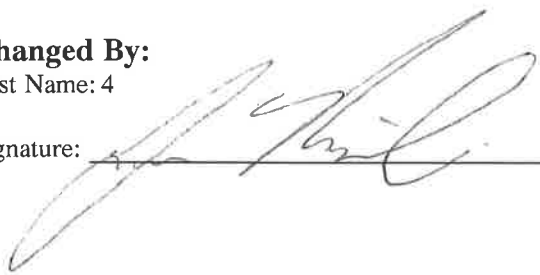

#116

Badge No.: 116

Date: 07/17/2019