

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSA-0031
Location:	STAFFORD TOWNSHIP P.D.	
Calibration File No.:	01536	Calib. Date: 09/13/2019
Certification File No.:	01537	Calib. No.: 00035
Linearity File No.:	01538	Cert. Date: 09/13/2019
Solution File No.:	01545	Cert. No.: 00030
Sequential File No.:	01545	Lin. Date: 09/13/2019
		Lin. No.: 00030
		Soln. Date: 10/11/2019
		Soln. No.: 00223
		File Date: 10/11/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0015
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 0580

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:00D		
Control 1 EC	0.099%	06:01D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	06:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:01D		
Control 2 EC	0.098%	06:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:03D		
Control 3 EC	0.098%	06:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NICCOLI

First Name: JOSEPH

MI: R

Signature: _____

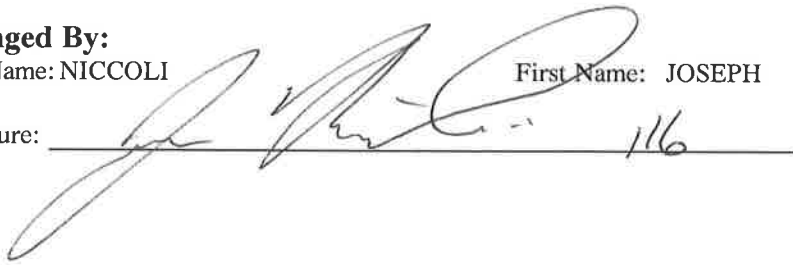

Badge No.: 116

Date: 10/11/2019